


HPLC Analysis for V2532901 Metenkefalin

Data file: D:\CHEM32\1\DATA\240215\601512 24021501Final.D
 Sample name: 601512 24021501Final
 Description: Mobile phase: Buffer A: 0.1% TFA in H₂O
 Buffer B: 0.1% TFA in ACN
 Gradient: 19-29% B in 20min, Flow rate: 1ml/min
 Column: Unitary C18, 4.6*150mm, 5um 100A
 Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 21
 Injection date: 2024/02/15 12:58:14 Injection: 1 of 1
 Last changed: 2024/02/15 14:59:59 Injection volume: 10.000
 Acq. operator: SYSTEM

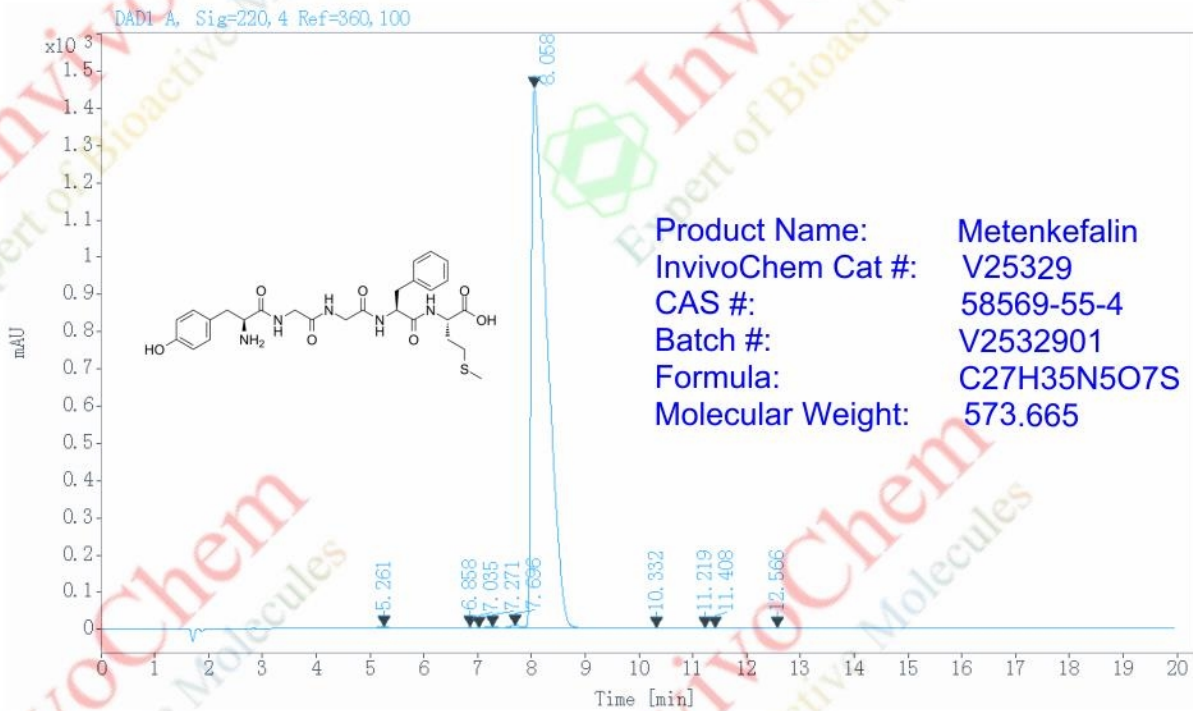

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area %	Name
5.261	BV R	0.1750	41.6511	3.4950	0.1409	
6.858	BV E	0.1452	5.3843	0.5552	0.0182	
7.035	VV E	0.0964	3.8599	0.5463	0.0131	
7.271	VV E	0.2168	23.2377	1.5511	0.0786	
7.696	VV E	0.1908	81.3785	6.3814	0.2752	
8.058	VB R	0.3058	29348.3848	1452.2419	99.2486	
10.332	BB	0.1968	10.4647	0.8098	0.0354	
11.219	BV	0.1979	16.0419	1.2162	0.0542	
11.408	VB	0.1871	13.7615	1.1062	0.0465	
12.566	BB	0.2490	26.4200	1.5970	0.0893	
	Sum		29570.5843			