


# HPLC Analysis for V1689201 TRV-120027

Data file: C:\CHEM32\1\DATA\250403\20250403 2025-04-03 08-59-19\602925  
25040303Final.D  
Sample name: 602925 25040303Final  
Description: Mobile Phase: Buffer A: 0.1% TFA in H2O  
Buffer B: 0.1% TFA in ACN  
Gradient: 13-23%B in 20min, Flow rate: 1.0ml/min  
Column: Unitary C18 5um 100A 4.6\*150mm  
Instrument: Agilent HPLC 1100  
Instrument: 1100 Location: 13  
Injection date: 2025/4/3 15:51:35 Injection: 1 of 1  
Last changed: 2025/4/3 11:40:40 Injection volume: 10.000

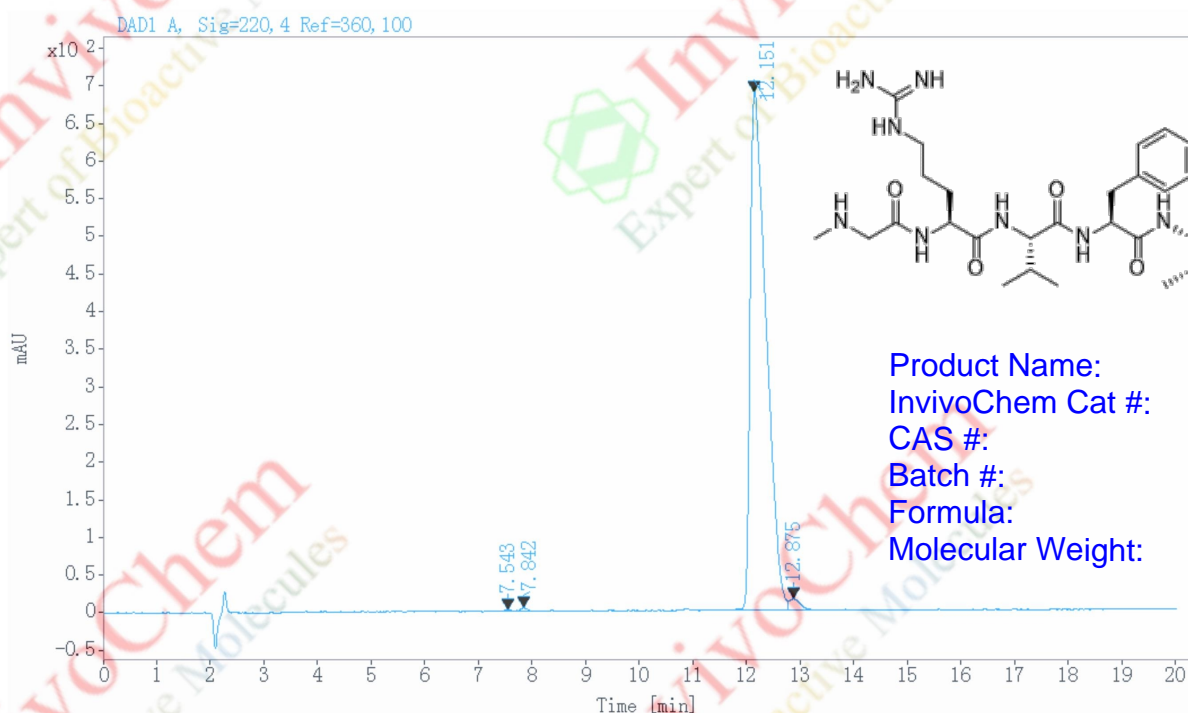

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
7.543	MF	0.2770	23.6620	1.4239	0.1625	
7.842	FM	0.1653	45.5627	4.5942	0.3129	
12.151	MF	0.3460	14286.9932	688.1001	98.1221	
12.875	FM	0.2283	204.1993	14.9065	1.4024	
	Sum		14560.4172			