



HPLC Analysis for V7701801 Fibrinogen-Binding Peptide TFA

Data file: D:\CHEM32\1\DATA\250416\603125 25041601Final.D
 Sample name: 603125 25041601Final
 Description: Mobile Phase: Buffer A: 0.1% TFA in H₂O
 Buffer B: 0.1% TFA in ACN
 Gradient: 8-18%B in 20min, Flow rate: 1.0ml/min
 Column: Unitary C18 5um 100A 4.6*150mm
 Instrument: Agilent HPLC 1100

Instrument: 1100
 Injection date: 2025/4/16 9:54:01
 Last changed: 2025/4/16 11:17:14

Location: 2
 Injection: 1 of 1
 Injection volume: 10.000
 Acq. operator: SYSTEM

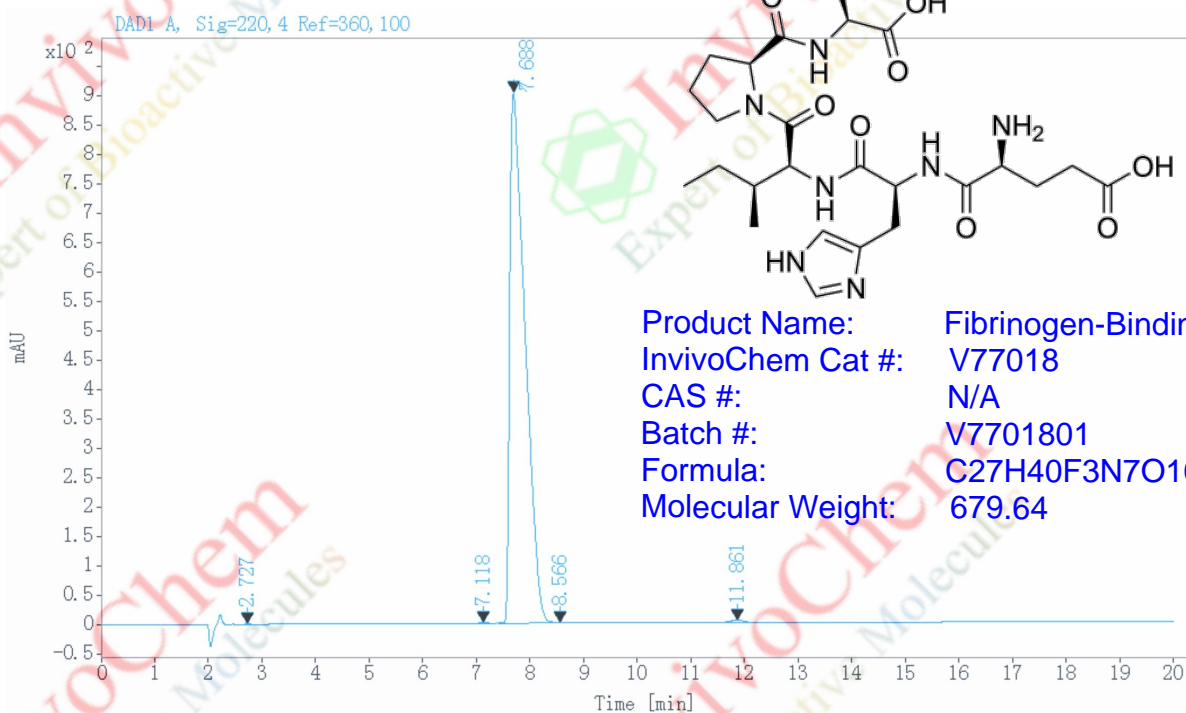

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area% Name
2.727	BB	0.0801	6.2335	1.2091	0.0347
7.118	MM	0.1642	3.3953	0.3447	0.0189
7.688	MF	0.3296	17864.3086	903.2314	99.4992
8.566	FM	0.1977	6.6725	0.5625	0.0372
11.861	BB	0.2784	73.6159	4.0062	0.4100
Sum			17954.2258		