


HPLC Analysis for V3232201 Zegocractin (CM-4620)

=====

Acq. Operator	: SYSTEM	Seq. Line	: 14
Acq. Instrument	: 12601c	Location	: Vial 26
Injection Date	: 06/03/2025 5:22:21 PM	Inj	: 1
		Inj Volume	: 2.000 µl
Acq. Method	: C:\CHEM32\1\DATA\FCOMPOUND\TEST 2025-06-03 12-16-09\TEST12.M		
Analysis Method	: C:\CHEM32\1\DATA\FCOMPOUND\TEST 2025-06-03 12-16-09\TEST12.M (Sequence Method)		

=====

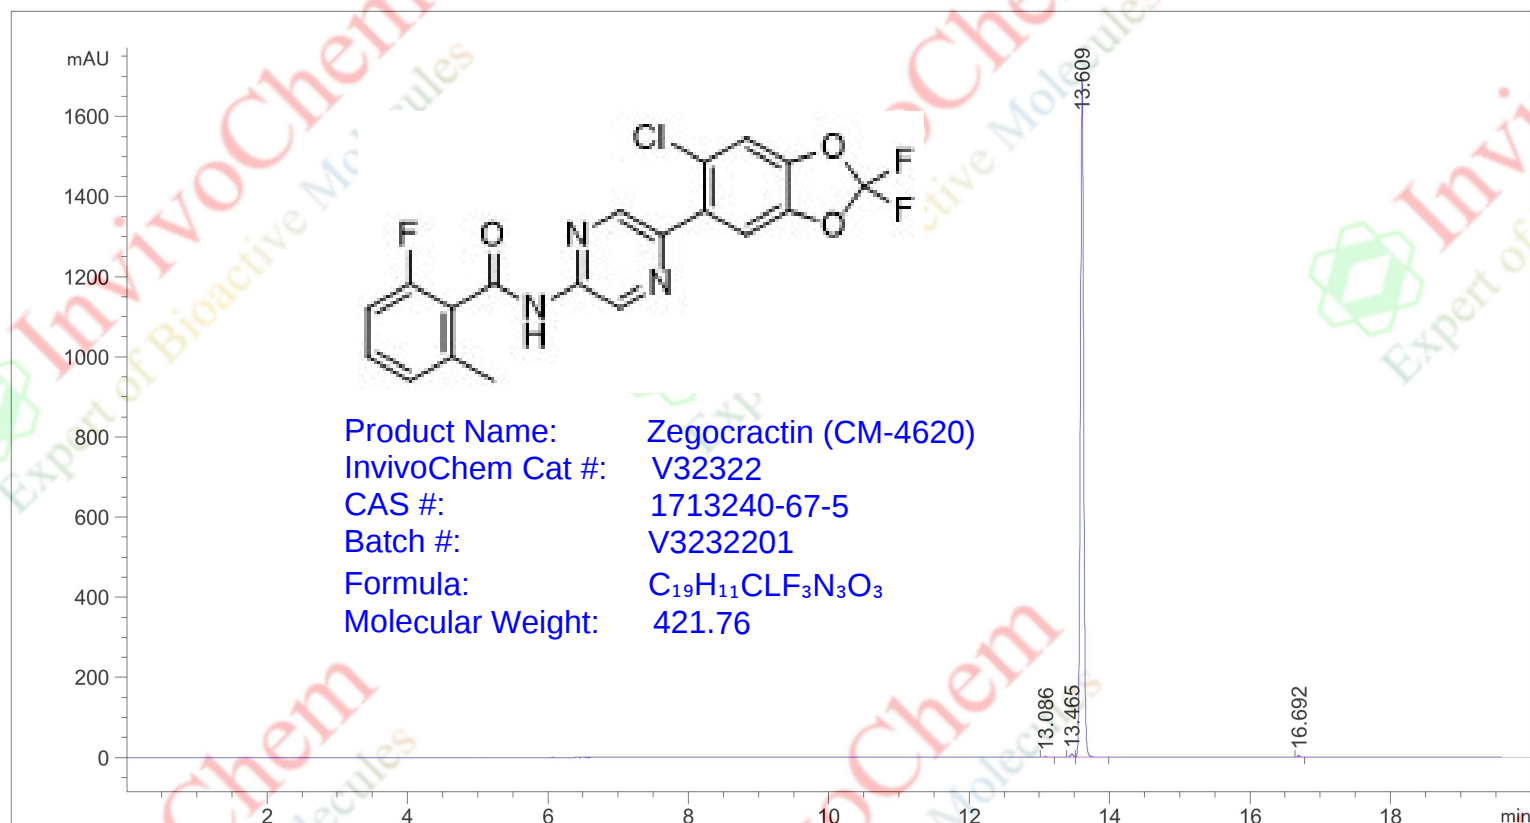

Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=325,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	13.086	BB	0.0566	5.96498	1.59736	0.1085
2	13.465	BV	0.0504	25.90741	7.98201	0.4712
3	13.609	VB	0.0497	5456.10400	1687.22644	99.2302
4	16.692	BB	0.0375	10.45543	4.27549	0.1902

Totals : 5498.43182 1701.08130

=====
*** End of Report ***