


# HPLC Analysis for V3712701 Deslorelin Acetate

Data file: D:\CHEM32\1\DATA\250321\800008 25020180Final.D  
Sample name: 800008 25020180Final  
Description: Mobile Phase: Buffer A: 0.1% TFA in H<sub>2</sub>O  
Buffer B: 0.1% TFA in ACN  
Gradient: 27-37%B in 20min, Flow rate: 1.0ml/min  
Column: Unitary C18 5um 100A 4.6\*150mm  
Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 66  
Injection date: 2025/3/21 13:19:31 Injection: 1 of 1  
Last changed: 2025/3/21 12:35:32 Injection volume: 5.000  
Acq. operator: SYSTEM

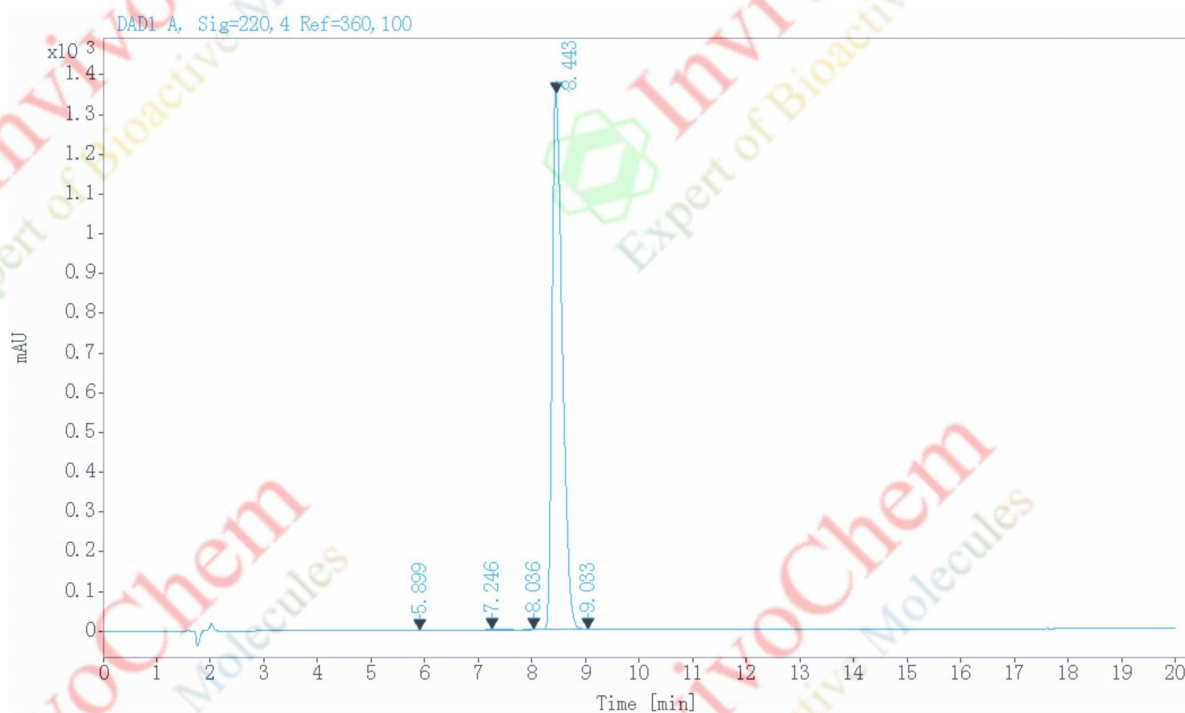

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area %	Name
5.899	BB	0.1260	4.9535	0.6423	0.0273	
7.246	MM	0.3052	58.2701	3.1825	0.3208	
8.036	MF	0.2020	5.5887	0.4611	0.0308	
8.443	FM	0.2227	18077.2324	1353.1851	99.5276	
9.033	FM	0.1459	16.9876	1.9402	0.0935	
Sum			18163.0323			

