

HPLC Analysis for V254001 740 Y-P (PDGFR 740Y-P)

Data file: D:\CHEM32\1\DATA\230526\20230526_2023-05-26_14-46-56\602620
23052508Final-004.D


Sample name: 602620 23052508Final

Description: Mobile phase: Buffer A: 0.1% TFA in H₂O
Buffer B: 0.1% TFA in ACN
Gradient: 21-31% B in 20min, Flow rate: 1.0ml/min
Column: Unitary C4, 4.6*150mm, 5um 100A
Instrument: Agilent HPLC 1100

Instrument: 1100 Location: 6

Injection date: 2023/5/26 16:07:32 Injection: 1 of 1

Last changed: 2023/5/26 16:27:58 Injection volume: 10.000
Acq. operator: SYSTEM

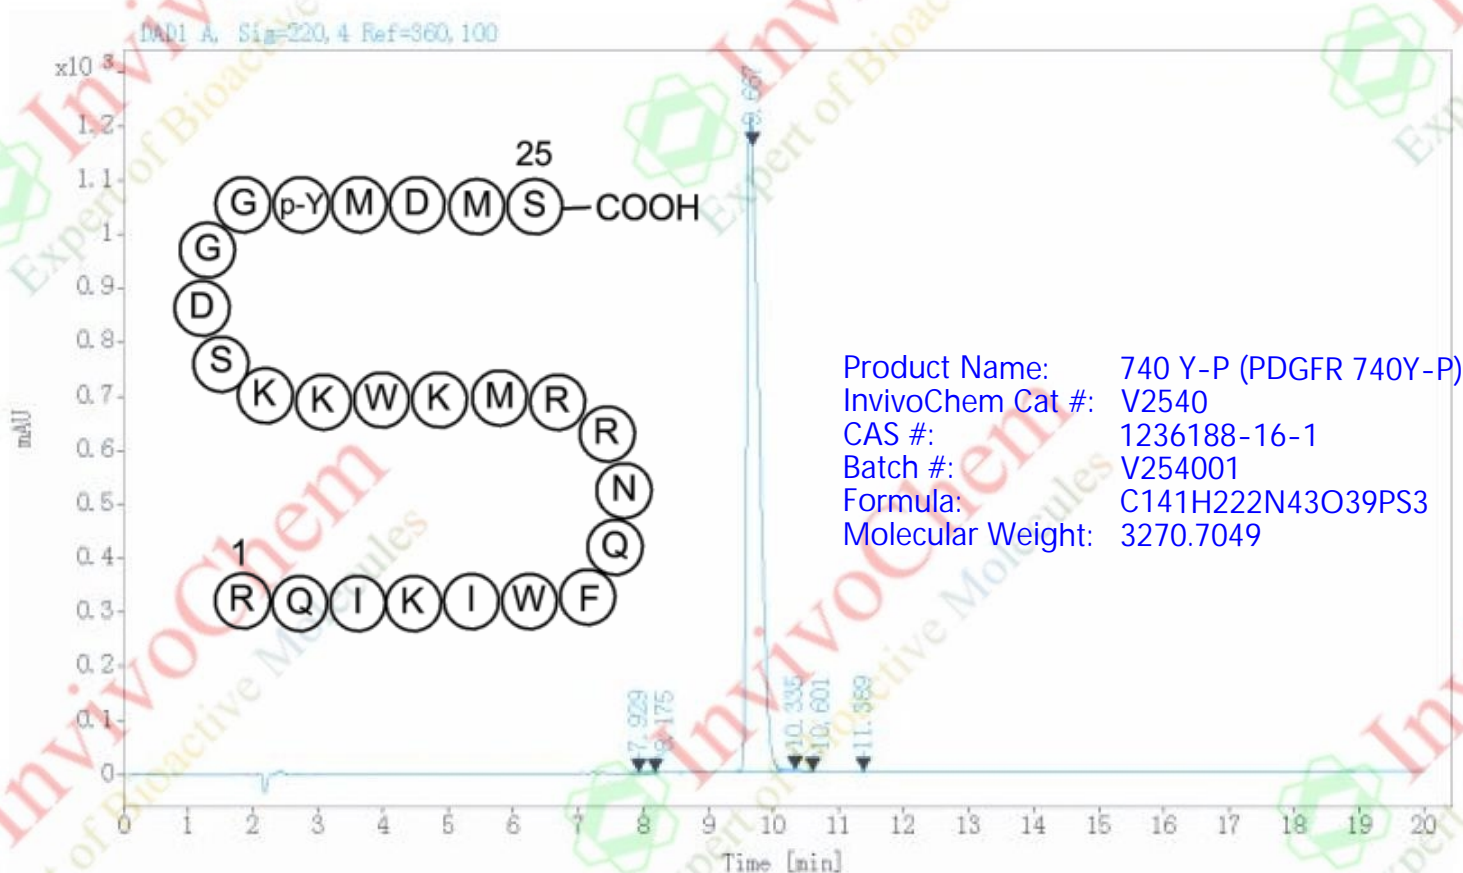

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT[min]	Type	Width[min]	Area	Height	Area%	Name
7.929	BV	0.2024	18.7575	1.4948	0.1170	
8.175	VBAB	0.1713	10.2679	0.8602	0.0640	
9.667	BV R	0.2154	15803.1816	1156.5216	98.5701	
10.335	VV E	0.3027	150.1520	6.8771	0.9366	
10.601	VB E	0.1850	32.0659	2.4454	0.2000	
11.389	BB	0.1533	17.9985	1.9941	0.1123	
	Sum		16032.4235			