


HPLC Analysis for V6449601 Pyr-Arg-Thr-Lys-Arg-AMC TFA

Data file: D:\CHEM32\1\DATA\231106\20231106 2023-11-06 11-26-21\605245
23100055Final.D
Sample name: 605245 23100055Final
Description: Mobile phase: Buffer A: 0.1% TFA in H₂O
Buffer B: 0.1% TFA in ACN
Gradient: 12-22% B in 20min, Flow rate: 1.0ml/min
Column: Unitary C18, 4.6*150mm, 5um 100A
Instrument: Agilent HPLC 1100
Instrument: 1100
Injection date: 2023/11/6 11:59:28
Last changed: 2023/11/6 12:40:09

Location: 36
Injection: 1 of 1
Injection volume: 10.000
Acq. operator: SYSTEM

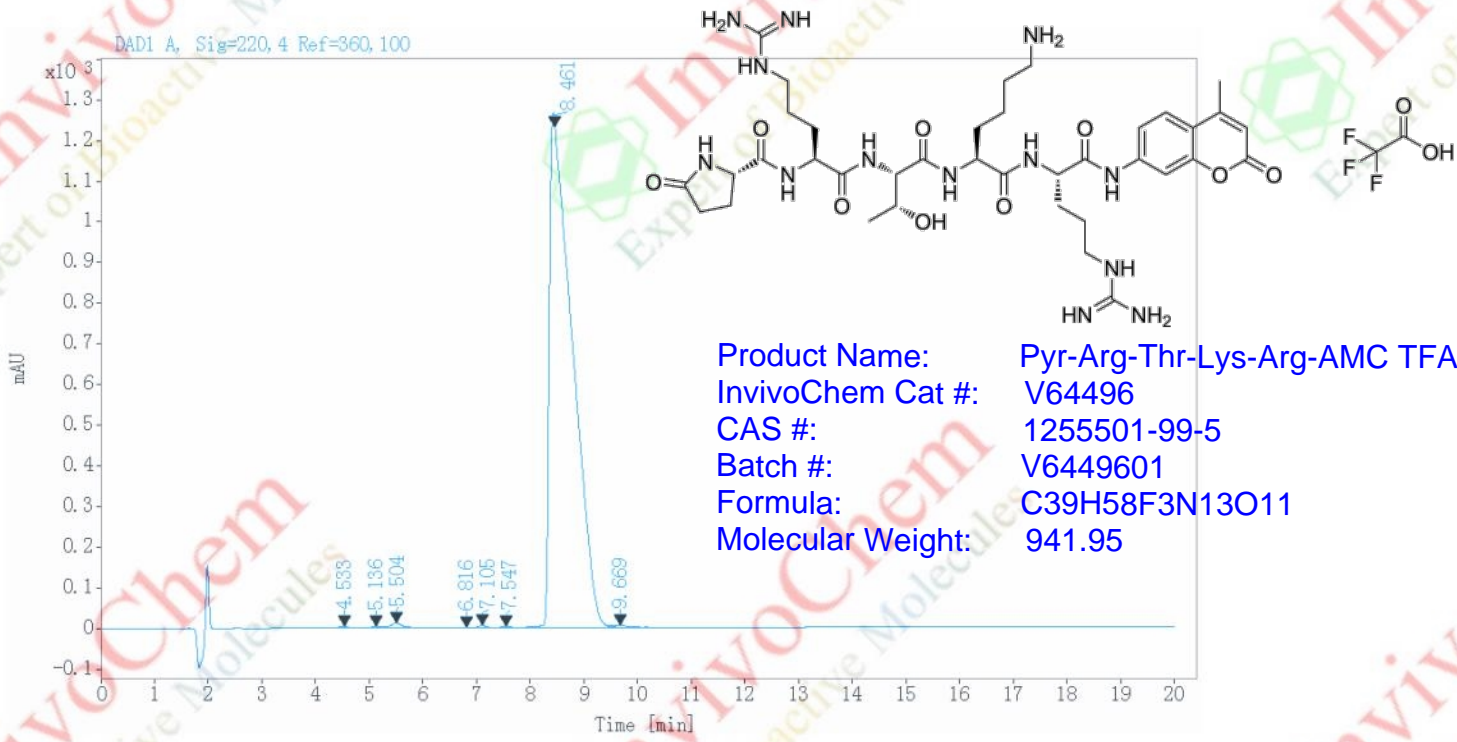

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area % Name
4.533	BB	0.1697	14.7193	1.4114	0.0393
5.136	BV E	0.2393	32.2696	1.9684	0.0863
5.504	VB R	0.2124	142.8363	10.6524	0.3818
6.816	BB F	0.1717	5.7289	0.5074	0.0153
7.105	BB	0.1625	47.4285	4.8323	0.1268
7.547	BB	0.1901	26.9848	2.3471	0.0721
8.461	BV R	0.4831	37039.9922	1217.0356	99.0039
9.669	VBAE	0.2936	102.6898	5.0430	0.2745
	Sum		37412.6494		