


HPLC Analysis for V3639801 Cecropin P1

Data file: D:\CHEM32\1\DATA\231216\601131 22110097 Final.D
 Sample name: 601131 22110097 Final
 Description: Mobile phase: Buffer A: 0.1% TFA in H₂O
 Buffer B: 0.1% TFA in ACN

Gradient: 31-41% B in 20 min, Flow rate: 1 ml/min
 Column: Unitary C18, 4.6*150 mm, 5 µm 100A
 Instrument: Agilent HPLC 1100

Instrument: 1100
 Injection date: 2023/12/16 16:02:49
 Last changed: 2023/12/16 15:30:07

Location: 81
 Injection: 1 of 1
 Injection volume: 20.000
 Acq. operator: SYSTEM

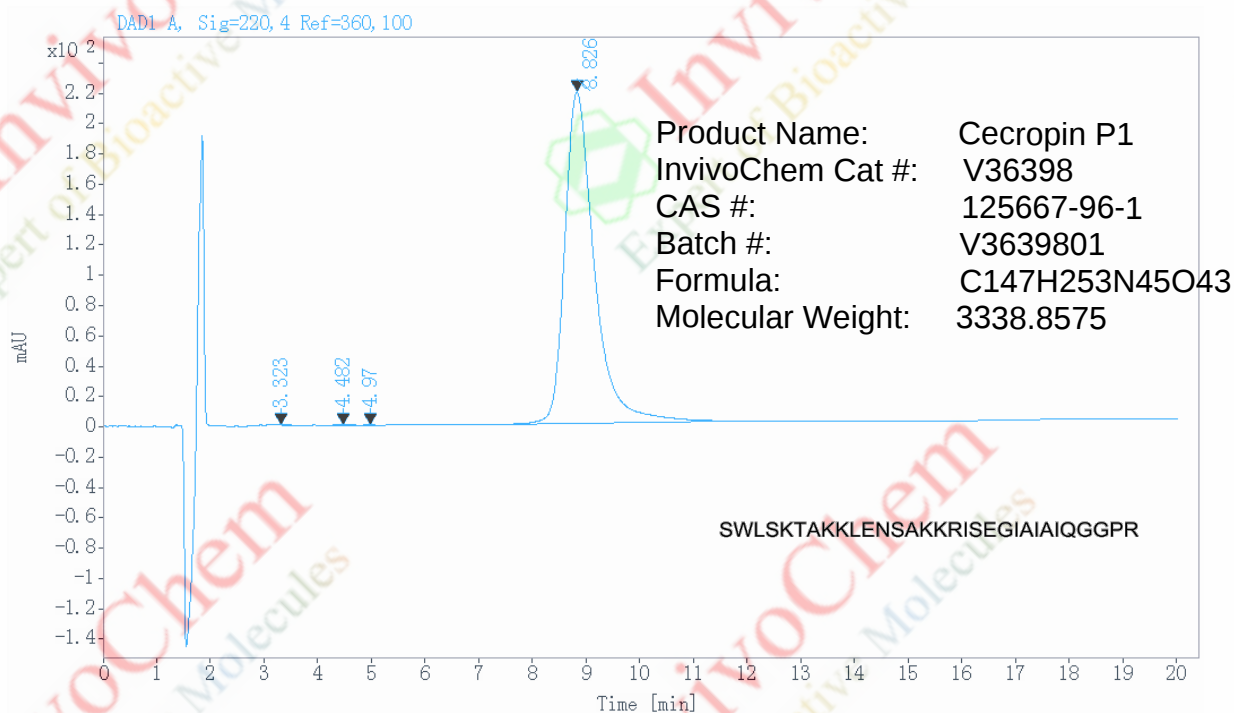

Signal: DAD1 A, Sig=220, 4 Ref=360, 100

RT [min]	Type	Width [min]	Area	Height	Area%	Name
3.323	MM	0.2180	6.0827	0.4651	0.0723	
4.482	MM	0.2964	13.5493	0.7620	0.1610	
4.970	MM	0.1769	4.1856	0.3943	0.0497	
8.826	BV R	0.5758	8390.0957	218.5855	99.7169	
Sum			8413.9134			