HPLC Analysis for V17405 C25-140 CAS#1358099-18-9

Sample Name: C25-140

Acq. Operator : SYSTEM Seq. Line : 2
Acq. Instrument : 1260lc Location : Vial 73

Inj Volume : 2.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.500 µl

Additional Info : Peak(s) manually integrated

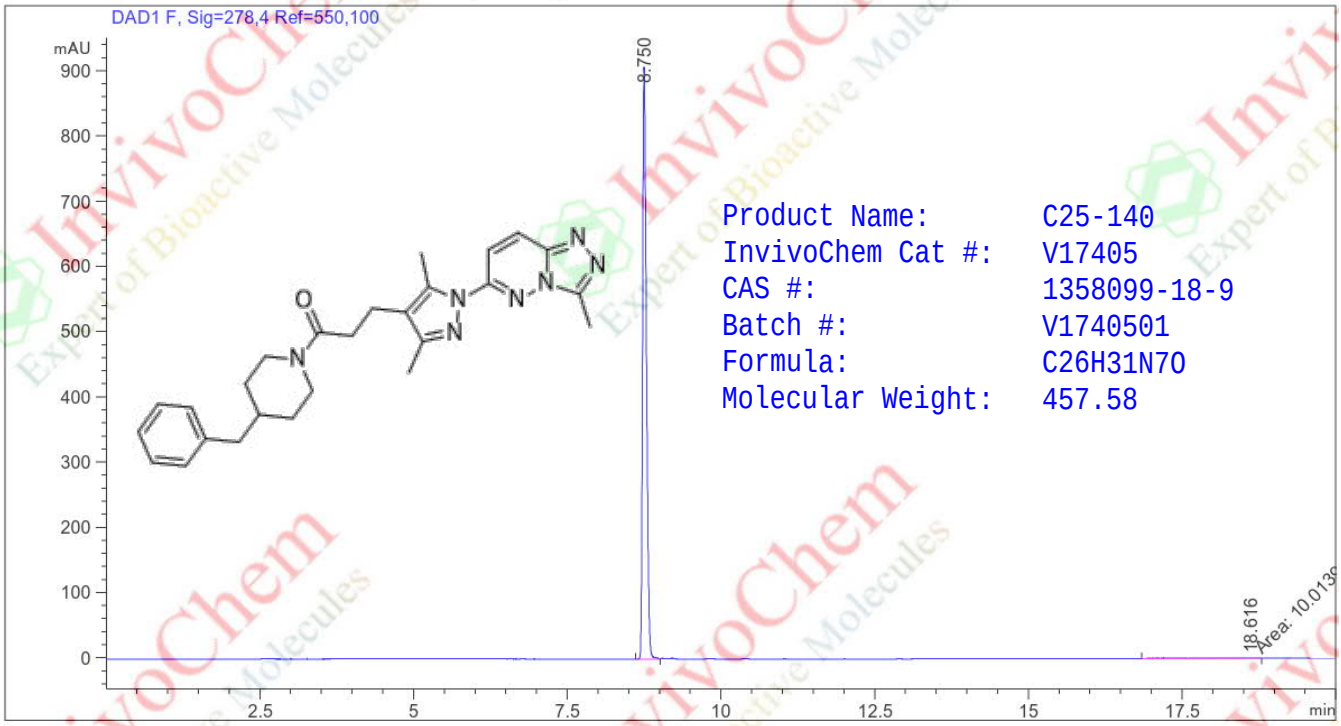

Area Percent Report

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 F, Sig=278,4 Ref=550,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.750	BV	0.0658	3874.19312	907.92200	99.0187
2	18.616	MM	0.3203	10.01385	5.21052e-1	0.9813
Totals :				3884.20697	908.44305	