


V8005 QLT0267 HPLC

Injection Date : 7 Sep 20
Sample Name : 6975-75-3
Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5% increase to 95%B within 7.5 min, 95%B for 7.5 min.
Flow Rate: 1.0ml/min
Column:Sunfire C18,4.6*150mm,3.5um
Column Temperature: 45 C
Detection:UV(214,4nm) and MS(ESI,Pos mode,110 to 1500 amu)

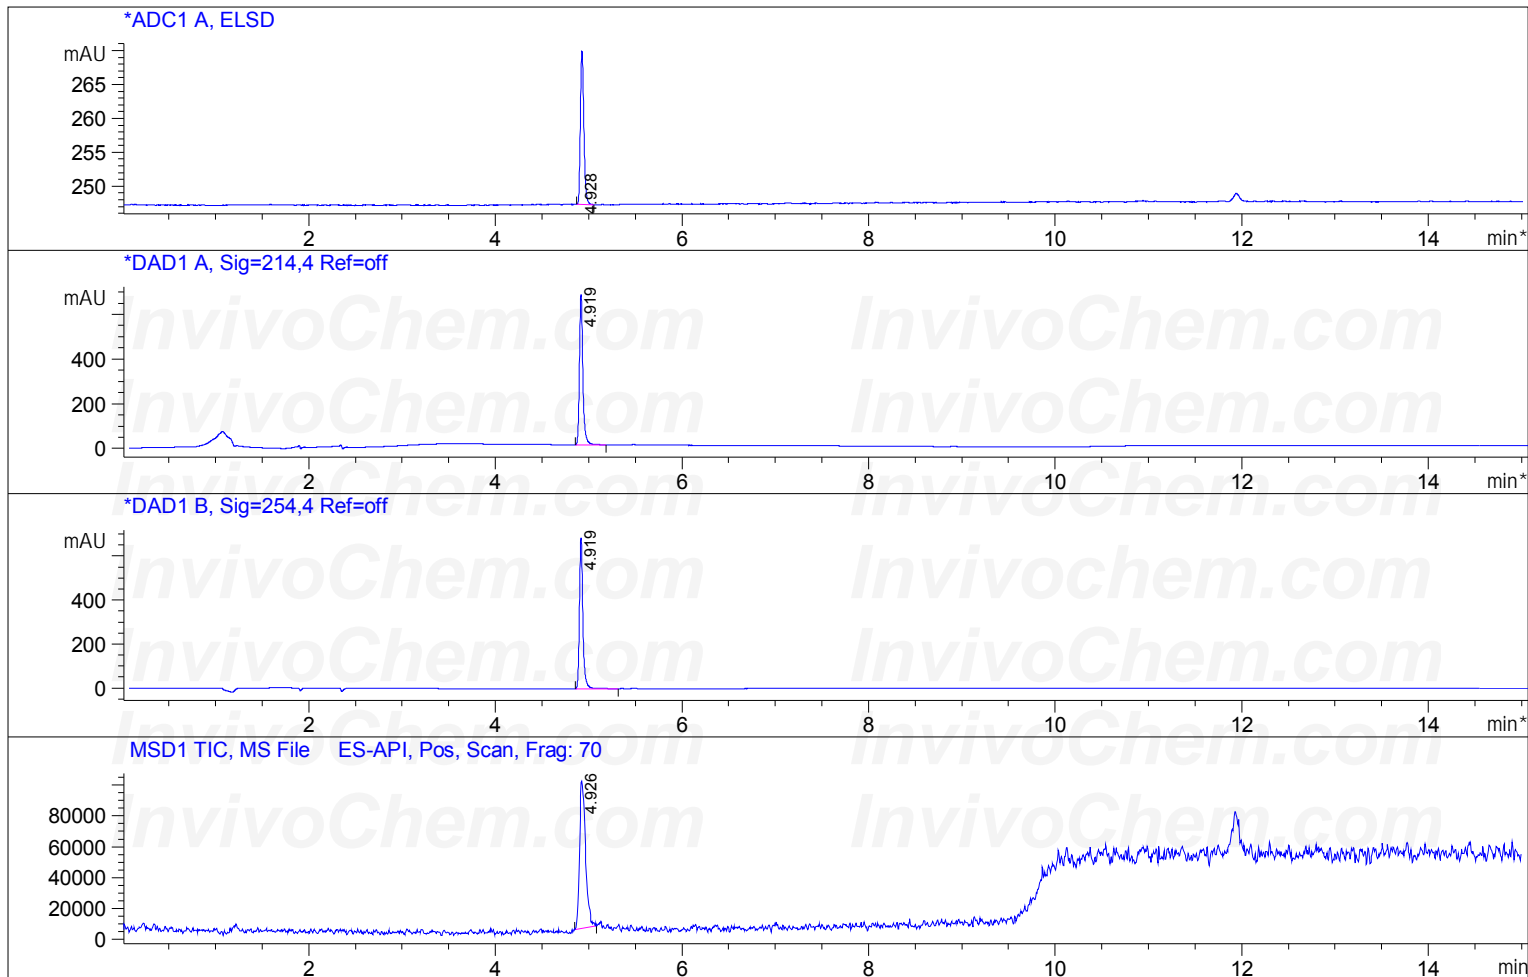

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
4.93	0.04	57.88	22.66	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
4.92	0.04	1700.29	673.65	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
4.92	0.04	1740.29	687.63	100.00