

1. Analysis Information

Product Name: EUK 134
Operator: David
Injection Date: 6/23/2016 12:46:52 AM
Batch No.: 1


2. HPLC Condition

Column: Athena C18, 3 μ m, 2.1mm $\times$ 100 mm
Solvent A: 0.1% H₃PO₄ in 100% Acetonitrile
Solvent B: 0.1% H₃PO₄ in 100% Water

Gradient:	Time	A	B
	0.0min	10%	90%
	6.0min	95%	5%
	10.0min	95%	5%
	10.0min	Stop	Stop

Flow rate: 0.5ml/min
Wavelength: 230nm
Volume: 3.0 μ l

3. Result

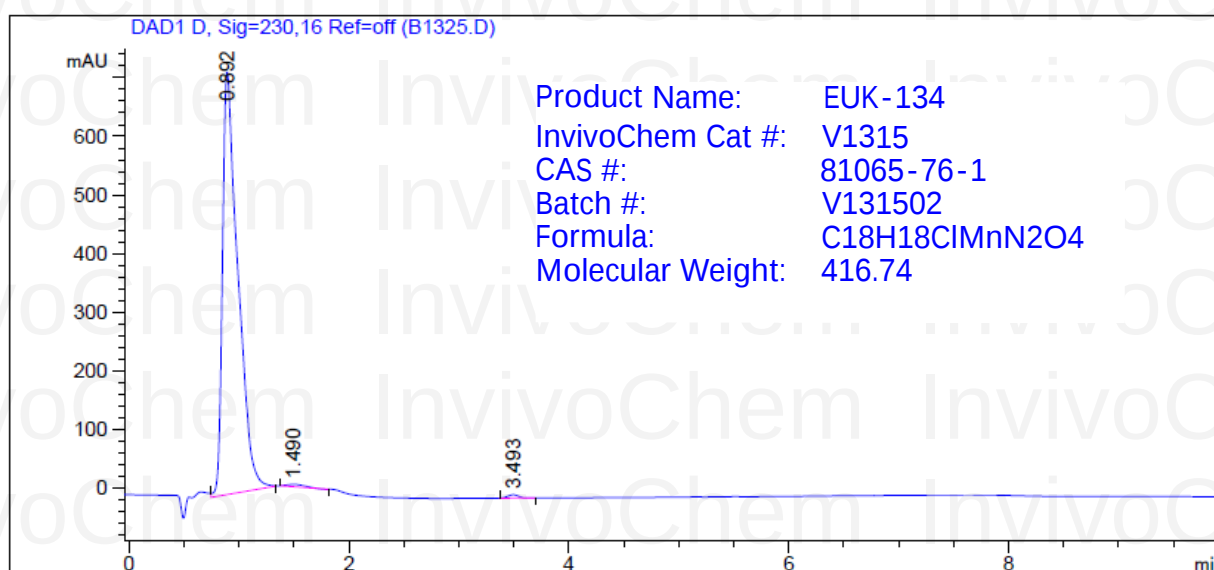

Rank	RetTime(min)	Area(mAU*s)	Area %
1	0.892	7005.82813	98.8489
2	1.490	46.63623	0.6580
3	3.493	34.94359	0.4930