


MASS SPECTROMETRY REPORT

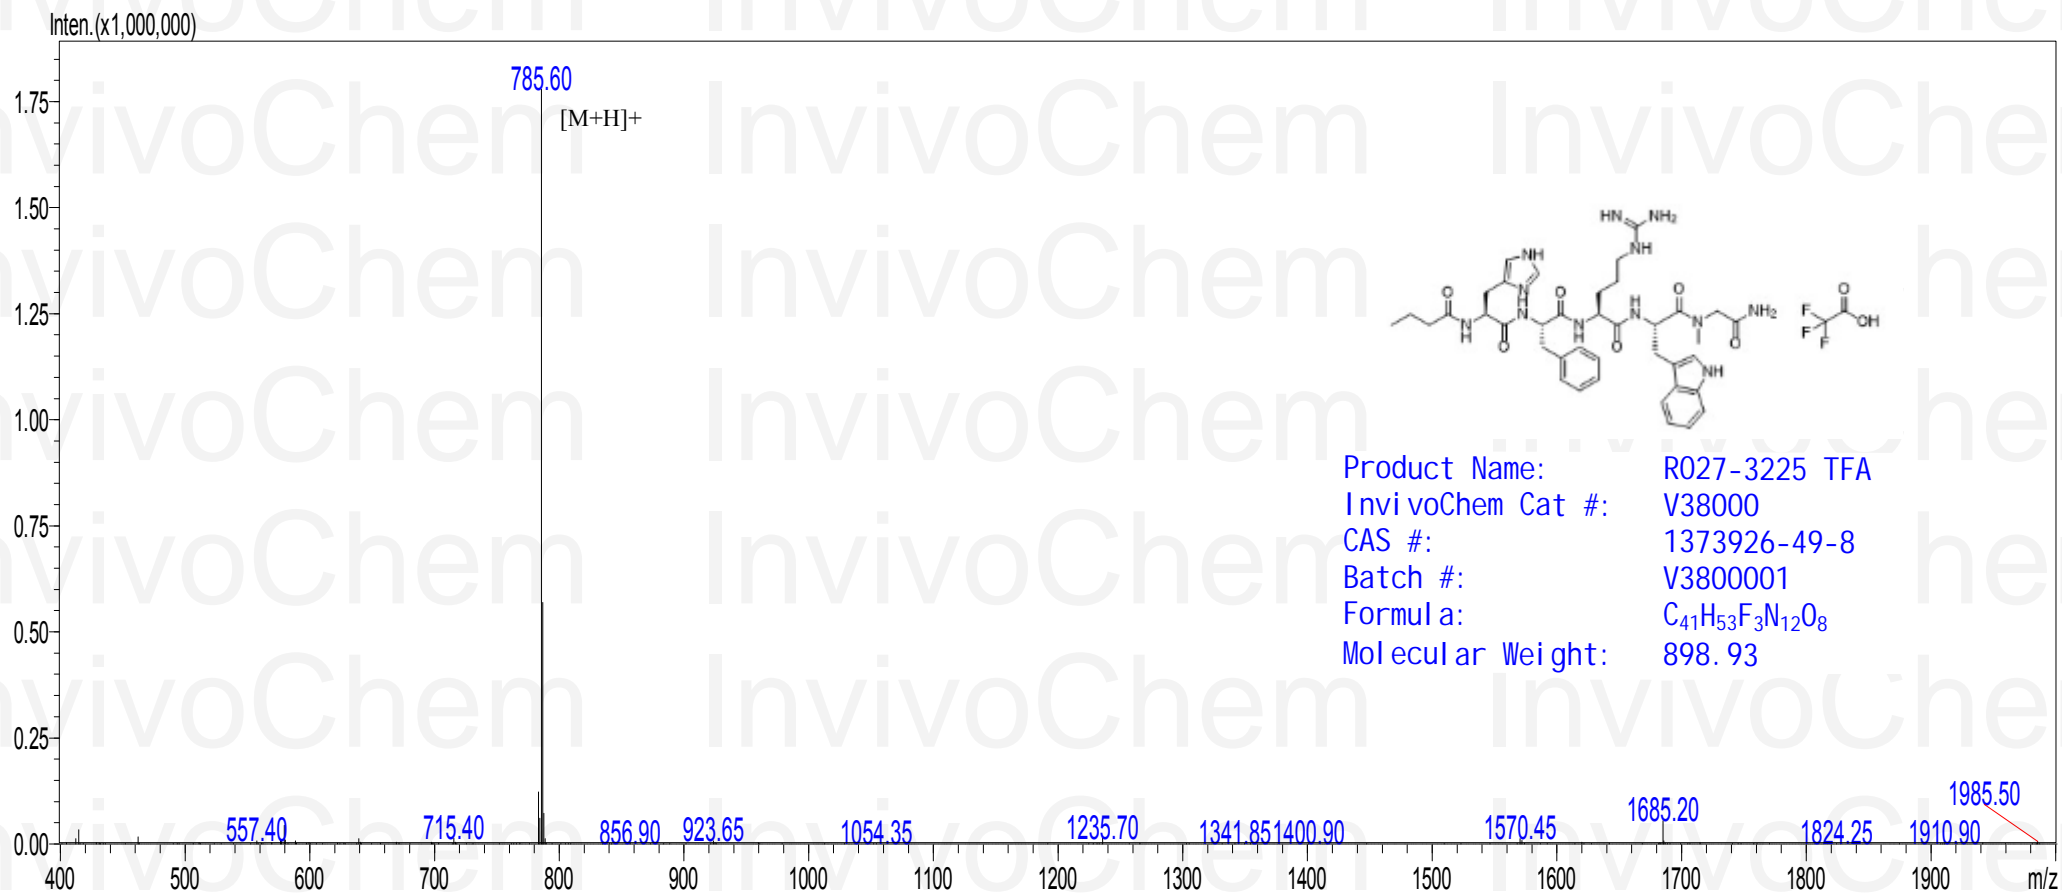

Sample Description

Analyzed date: 2021-3-18
 Analyst: SHAO
 Sample: 603246
 M.W.: 784.9
 Lot. No.:

Instrument

Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250°C
 Block Temp.: 200°C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv
 Detector: 1.5kv
 T. Flow: 0.2ml/min
 B. Conc.: 50%H₂O/50%ACN