


LCMS Analysis for V6449601 Pyr-Arg-Thr-Lys-Arg-AMC TFA

MASS SPECTROMETRY REPORT

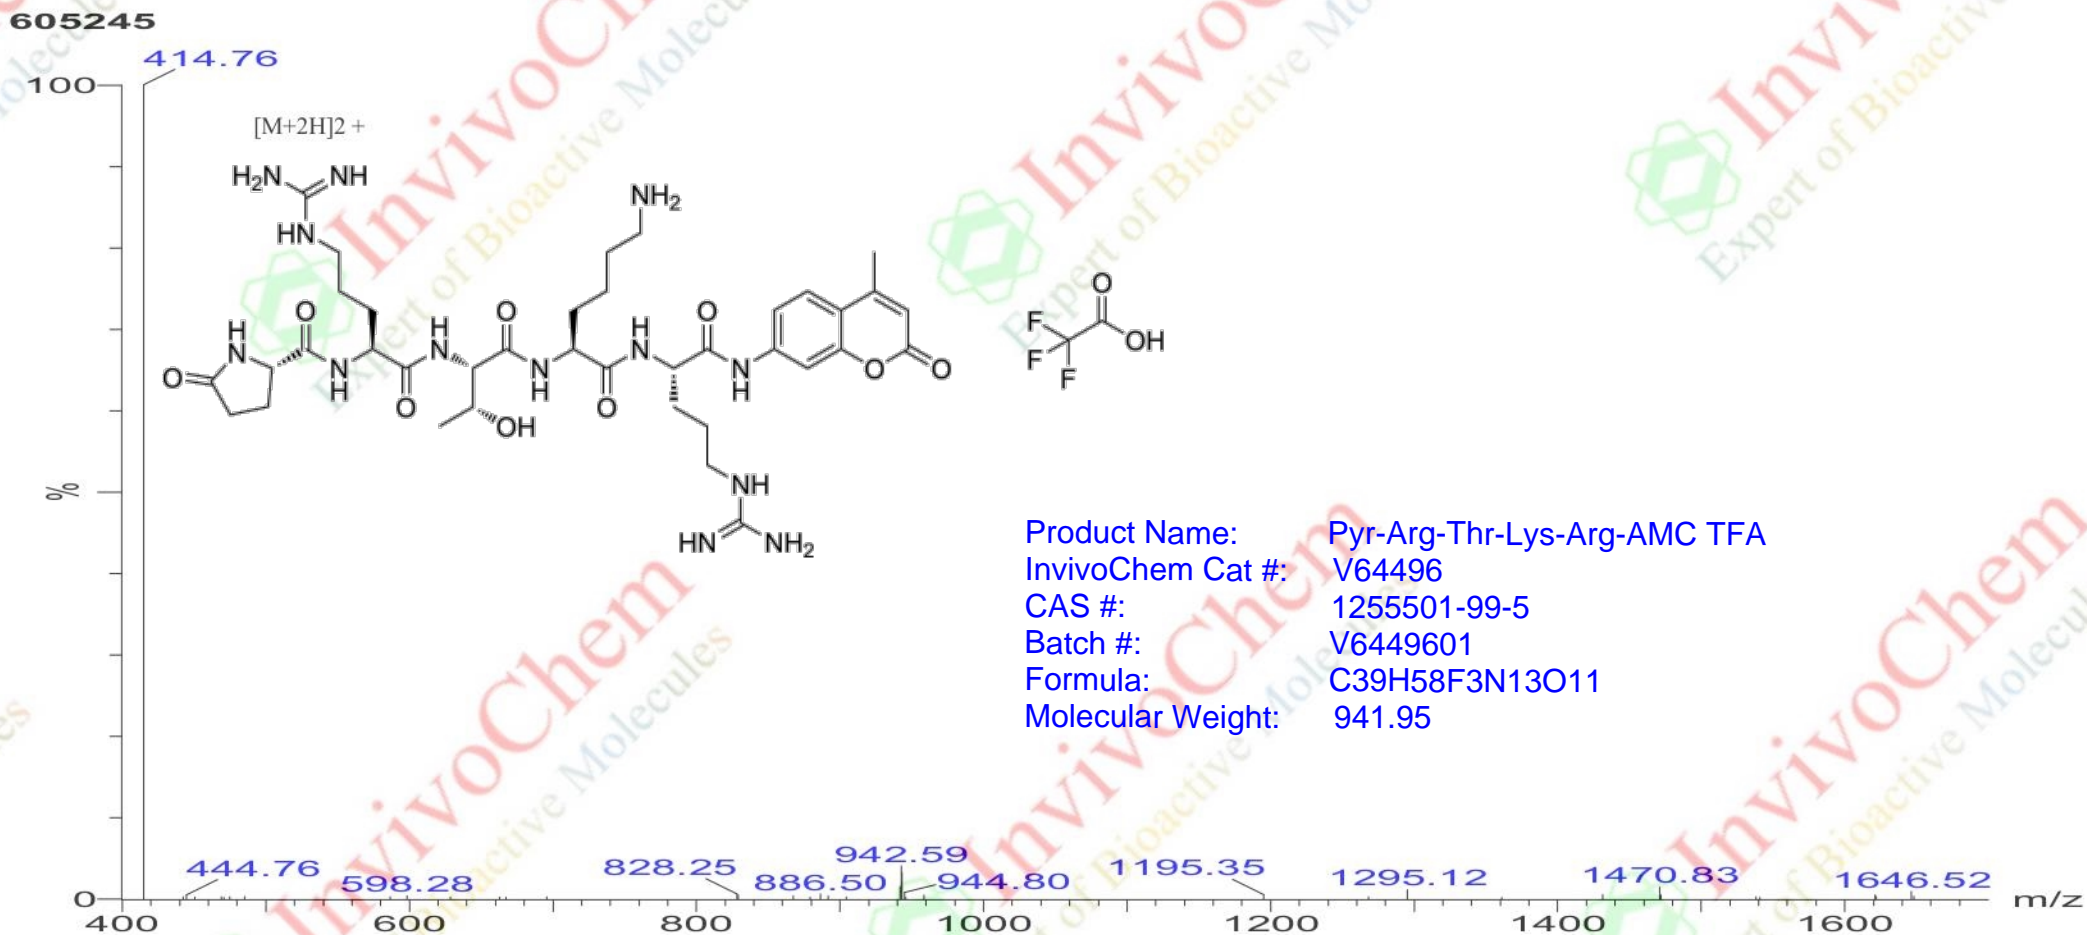

Sample Description

Analyzed date: 2023-11-06
 Analyst: SHAO
 Sample: 605245
 M.W.: 827.9
 Lot. No.:

Instrument

Waters 2695
 Probe: ESI
 Nebulizer Gas Flow: 1.5L/min
 CDL: -20.0v
 CDL Temp.: 250 °C
 Block Temp.: 200 °C

Probe Bias: +4.5kv
 Detector: 1.5kv
 T. Flow: 0.5ml/min
 B. Conc.: 50%H₂O/50%ACN