


LCMS Analysis for V5301201 LLO (91-99) (Listeriolysin O (91-99))

MASS SPECTROMETRY REPORT

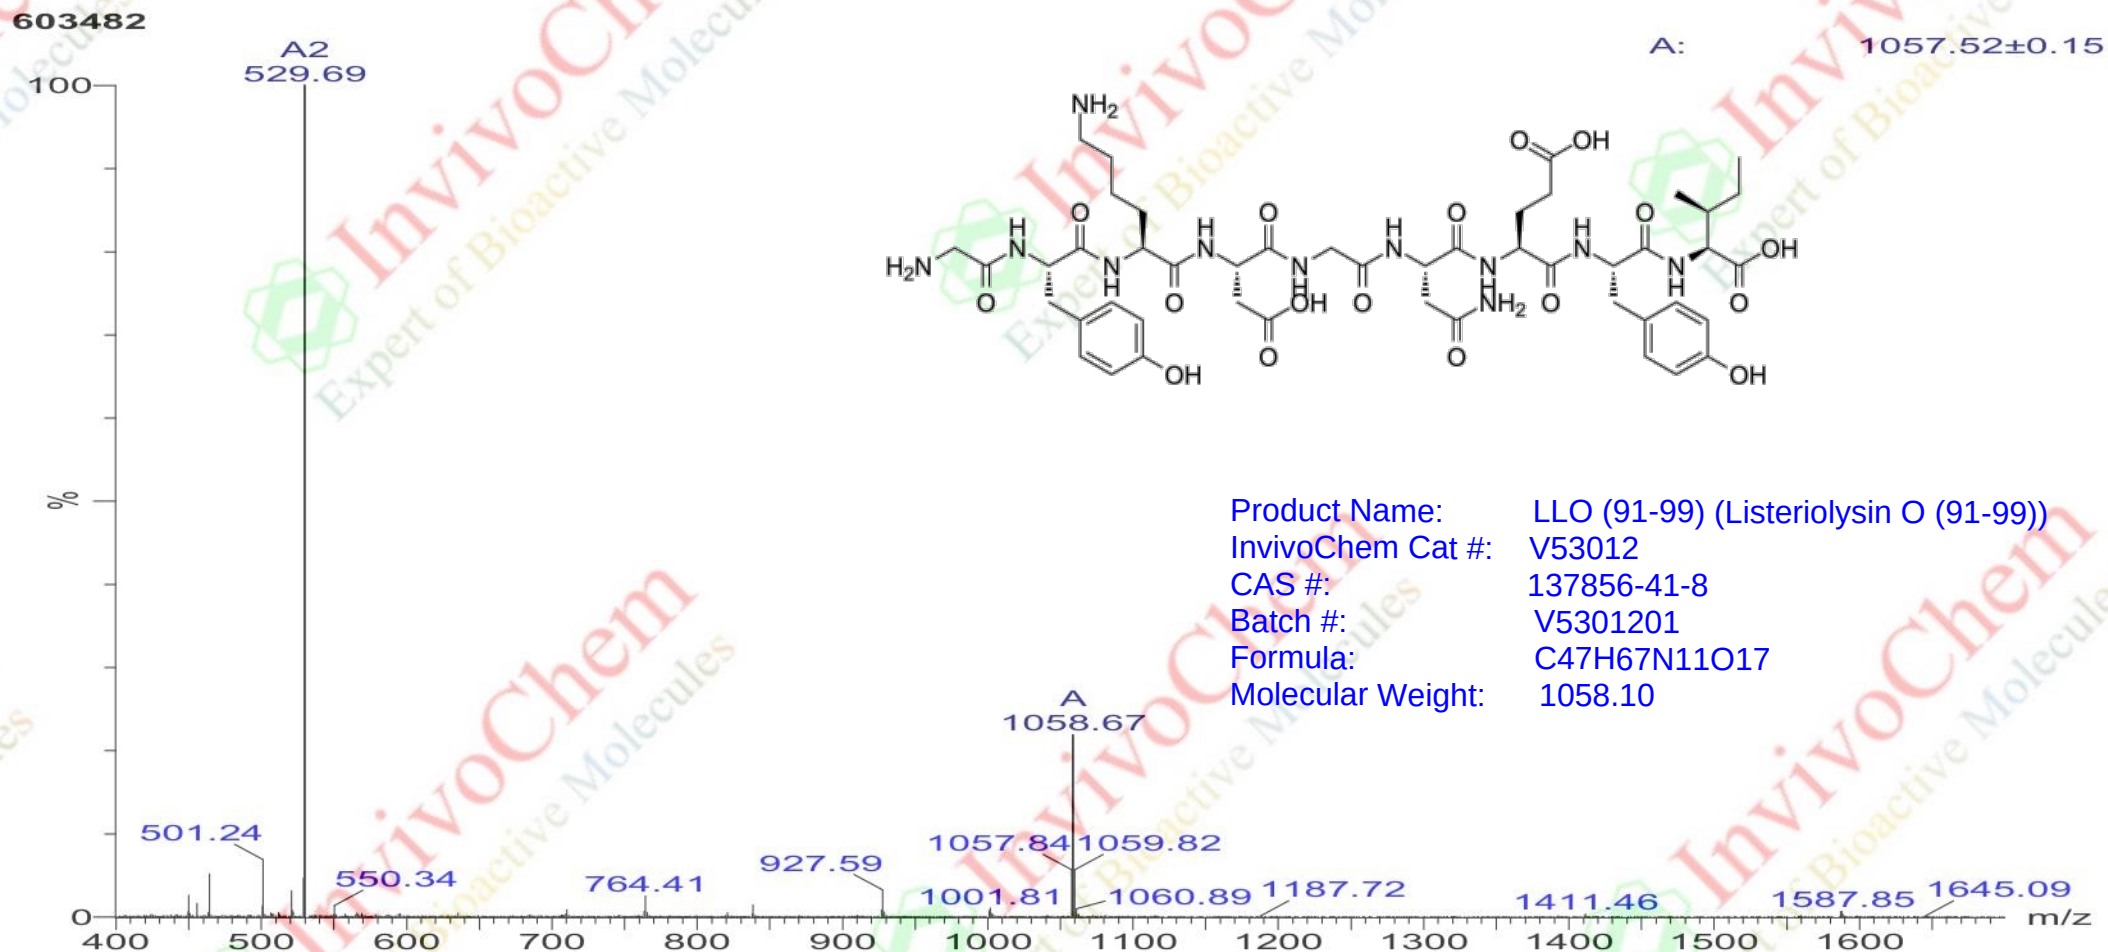

Sample Description

Analyzed date: 2023-02-24

Analyst: SHAO

Sample: 603482

M.W.: 1058.1

Lot. No.:

Instrument

Waters 2695

Probe:

ESI

Probe Bias:

+4.5kv

Nebulizer Gas Flow:

1.5L/min

Detector:

1.5kv

CDL:

-20.0v

T. Flow:

0.5ml/min

CDL Temp.:

250 °C

B. Conc.:

50%H₂O/50%ACN

Block Temp.:

200 °C