


MS Analysis for V3262601 LL-37, Human

MASS SPECTROMETRY REPORT

800072-24032101-02

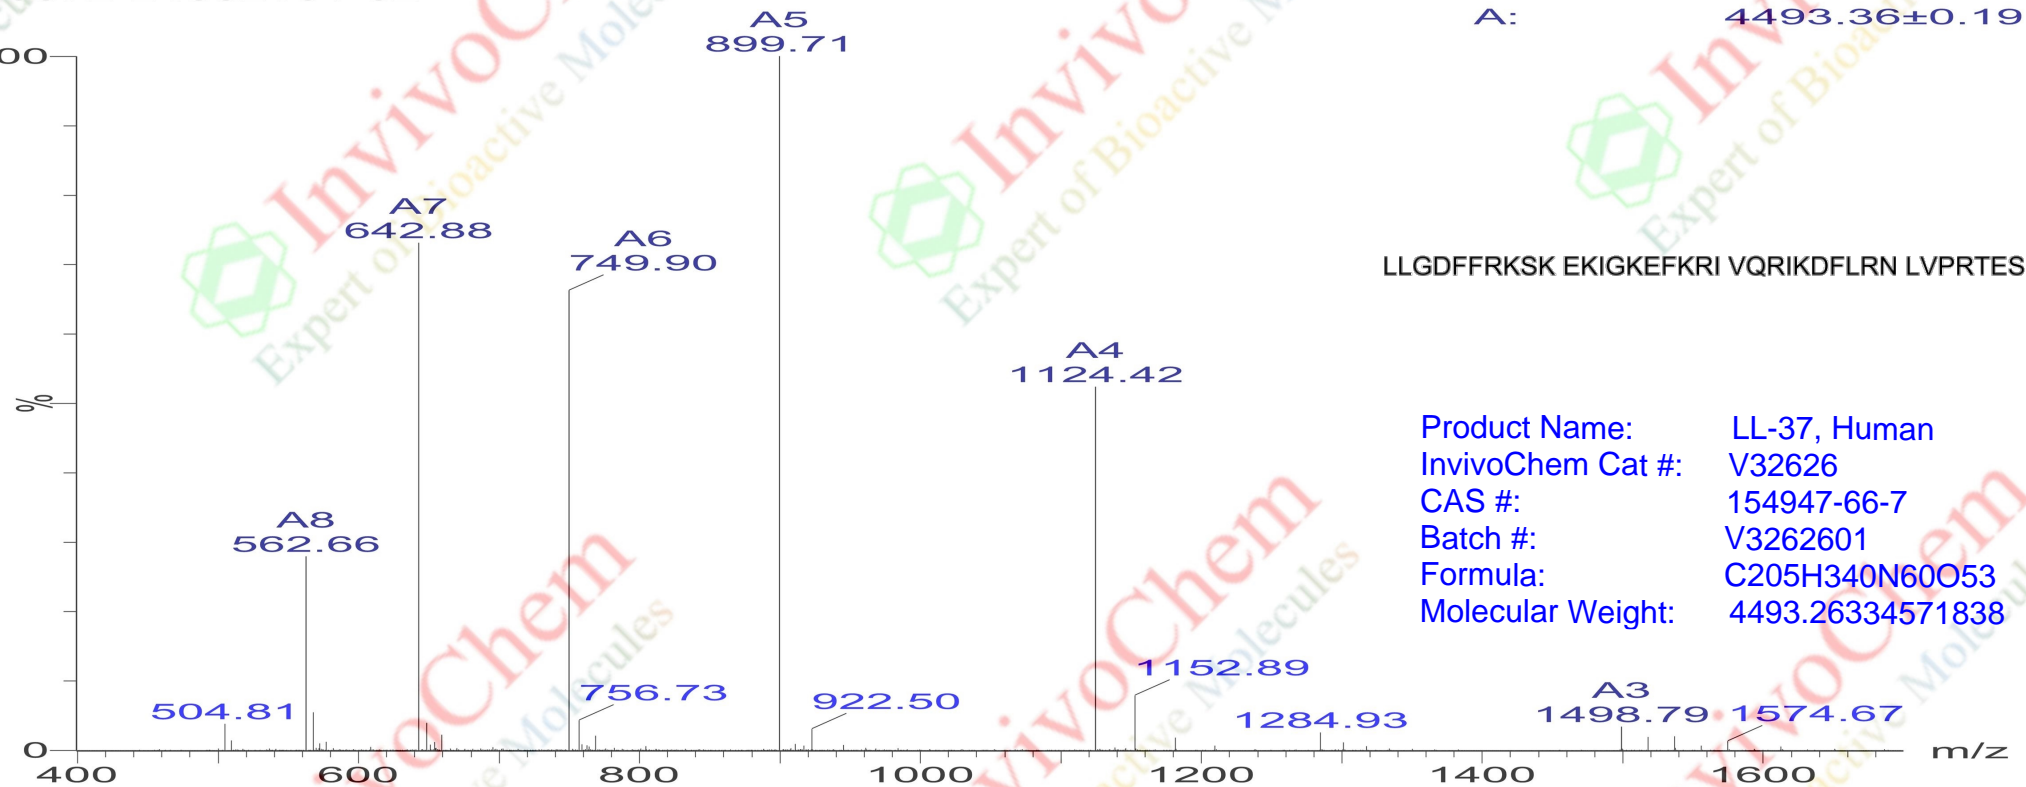

Sample Description

Analyzed date: 2024-07-01
Analyst: SHAO
Sample: 800072-24032101-02
M.W.: 4493.3
Lot. No.:

Instrument

Waters ZQ2000
Probe: ESI
Nebulizer Gas Flow: 10 L/min
CDL: 52.0v
CDL Temp.: 350 °C
Block Temp.: 120 °C

Probe Bias: +3.5kv
Detector: 0.05kv
T. Flow: 0.5ml/min
B. Conc.: 50%H2O/50%ACN